

# Echocardiography and pulse contour analysis to assess cardiac output in trauma patients

F. FRANCHI<sup>1</sup>, E. FALCIANI<sup>1</sup>, K. DONADELLO<sup>2</sup>, V. ZACÀ<sup>3</sup>, R. SILVESTRI<sup>1</sup>  
E. S. TACCONI<sup>2</sup>, L. CUBATTOLI<sup>1</sup>, P. MONGELLI<sup>1</sup>, P. GIOMARELLI<sup>1</sup>, S. SCOLLETTA<sup>1</sup>

<sup>1</sup>Department of Anesthesia and Intensive Care, University of Siena, Siena, Italy; <sup>2</sup>Department of Intensive Care, Erasme University Hospital; Université Libre de Bruxelles, Bruxelles, Belgium; <sup>3</sup>Department of Cardiovascular Disease, University of Siena, Siena, Italy

## ABSTRACT

**Background.** Echocardiography is a valuable technique to assess cardiac output (CO) in trauma patients, but it does not allow a continuous bedside monitoring. Beat-to-beat CO assessment can be obtained by other techniques, including the pulse contour method MostCare. The aim of our study was to compare CO obtained with MostCare (MC-CO) with CO estimated by transthoracic echocardiography (TTE-CO) in trauma patients.

**Methods.** Forty-nine patients with blunt trauma admitted to an intensive care unit and requiring hemodynamic optimization within 24 hours from admission were studied. TTE-CO and MC-CO were estimated simultaneously at baseline, after a fluid challenge and after the start of vasoactive drug therapy.

**Results.** One hundred sixteen paired CO values were obtained. TTE-CO values ranged from 2.9 to 7.6 L·min<sup>-1</sup>, and MC-CO ranged from 2.8 to 8.2 L·min<sup>-1</sup>. The correlation between the two methods was 0.94 (95% confidence interval [CI]=0.89 to 0.97; P<0.001). The mean bias was -0.06 L·min<sup>-1</sup> with limits of agreements (LoA) of -0.94 to 0.82 L·min<sup>-1</sup> (lower 95% CI, -1.16 to -0.72; upper 95% CI, 0.60 to 1.04) and a percentage error of 18%. Changes in CO showed a correlation of 0.91 (95% CI=0.87 to 0.95; P<0.001), a mean bias of -0.01 L·min<sup>-1</sup> with LoA of -0.67 to 0.65 L·min<sup>-1</sup> (lower 95% CI, -0.83 to -0.51; upper 95% CI, 0.48 to 0.81).

**Conclusion.** CO measured by MostCare showed good agreement with CO obtained by transthoracic echocardiography. Pulse contour analysis can complement echocardiography in evaluating hemodynamics in trauma patients. (*Minerva Anestesiologica* 2013;79:137-46)

**Keywords:** Cardiac output - Hemodynamics - Pulse wave analysis.

In trauma patients continuous cardiac output (CO) monitoring is crucial to detect abrupt hemodynamic changes and to avoid low output syndrome and tissue hypoperfusion.<sup>1</sup> Thermodilution (ThD) by means of a pulmonary artery catheter (PAC) is considered the gold standard method for the measurement of CO in clinical practice.<sup>2</sup> However, the lack of beat-to-beat analysis does not allow to measure any sudden hemodynamic changes with this technique.<sup>3</sup> Furthermore, the use of PAC has been questioned, due to possible complications associated with right heart catheterization.<sup>4</sup> Consid-

ering these two major concerns, thermodilution CO monitoring has been restricted in trauma patients only to selected conditions.<sup>4</sup>

Echocardiography is a validated and non-invasive technique, which has lately emerged as a first-line CO diagnostic device in trauma patients.<sup>1, 5</sup> However, it is operator-dependent and does not provide a continuous bedside CO monitoring.<sup>6</sup> Thus, different systems have been developed to allow beat-to-beat calculation of CO.<sup>3</sup> In particular, pulse contour methods (PCMs) have gained popularity as they are easy to use, less operator dependent and can

provide CO monitoring on a beat-to-beat basis.<sup>3</sup> MostCare (Vygon, Padua, Italy) is a PCM that does not need any type of calibration and that can compute CO from the analysis of the arterial pressure wave acquired at radial or femoral sites.<sup>7, 8</sup> This technology has been studied in several clinical and experimental settings,<sup>8-11</sup> but its value has never been investigated in trauma patients.

The aim of our study was to compare CO assessed with the MostCare system (MC-CO) with CO estimated by transthoracic echocardiography (TTE-CO) in trauma patients after Intensive Care Unit (ICU) admission and hemodynamic stabilization.

### Materials and methods

Forty-nine trauma patients admitted to a 7-bed university hospital mixed ICU were prospectively enrolled. Approval from the Institutional Review Board was obtained, along with written informed consent from patients or their legal representative.

Inclusion criteria were: 1) trauma within 24 hours from ICU admission; 2) need for hemodynamic optimization with volume loading and/or with vasoactive drugs, according to the attending physician's decision. Exclusion criteria were: less than 18 years of age, presence of cardiac arrhythmias, aortic regurgitation or stenosis and ascending aortic diseases documented by echocardiography (these factors affecting the reliability of the PCM) and poor quality of echocardiographic images. All patients were monitored with a radial artery catheter and a central venous catheter, as a standard procedure.<sup>9</sup>

After ICU admission, therapeutic decisions were taken by the physician in charge, according to local guidelines for the hemodynamic treatment of trauma patients.<sup>12</sup> Briefly, the choice of administering fluids and/or vasoactive drugs was established on: 1) the evidence of signs of inadequate tissue perfusion; 2) an integrated monitoring based on low mean arterial pressure (MAP), low central venous oxygen saturation, low central venous pressure (CVP), and high pulse pressure variation; and 3) the evaluation of poor left ventricular function (*i.e.*, left ven-

tricular ejection fraction <40%) by means of TTE (deta (Figure 1). Patients were all sedated, intubated and mechanically ventilated; the indications for endotracheal intubation were: head injury with Glasgow Coma Score (GCS) less than 9; respiratory insufficiency and severe psychomotor agitation in the unstable patient. Heart rate (HR), MAP, CVP, temperature, diuresis and peripheral arterial oxygen saturation (SaO<sub>2</sub>) were hourly recorded. Intracranial pressure (ICP) was monitored by external ventricular drainage in case of traumatic brain injury (TBI) and GCS <9.

### Echocardiography measurements

Echocardiographies were performed using a standard transthoracic probe (Phased Array Probe, PA 240, Esaote, Italy) and a dedicated unit (MyLab™ 70 Xvision, Esaote, Italy). All echocardiographies were performed by the same trained operator (V.Z.). Stroke volume was estimated using standard views and formula (*i.e.*, the product of the aortic valve area by the velocity time integral of aortic blood flow).<sup>13</sup> Afterwards, TTE-CO was calculated as the product of HR and stroke volume averaged over five consecutive stroke volume values. Cardiac output calculation was performed off-line and blindly to the MostCare results.

### MostCare measurements

The MostCare system was connected via a simple cable to the patient's monitoring system for the continuous recording of the radial arterial pressure waveform and the computation of CO. MostCare analyses the arterial signal using a sampling frequency of 1,000 Hz. The high-frequency sampling is of primary importance for the calculation of the arterial impedance and the correct measurement of pressures. After zeroing the arterial pressure-transducer system and before each CO measurement, the arterial waveform signal fidelity was checked using a fast flush test to assess the adequacy of the damping of the arterial shape.<sup>14</sup> In case of resonance effect of the catheter-transducer system, we adapted the MostCare's setting to maximise the signal-

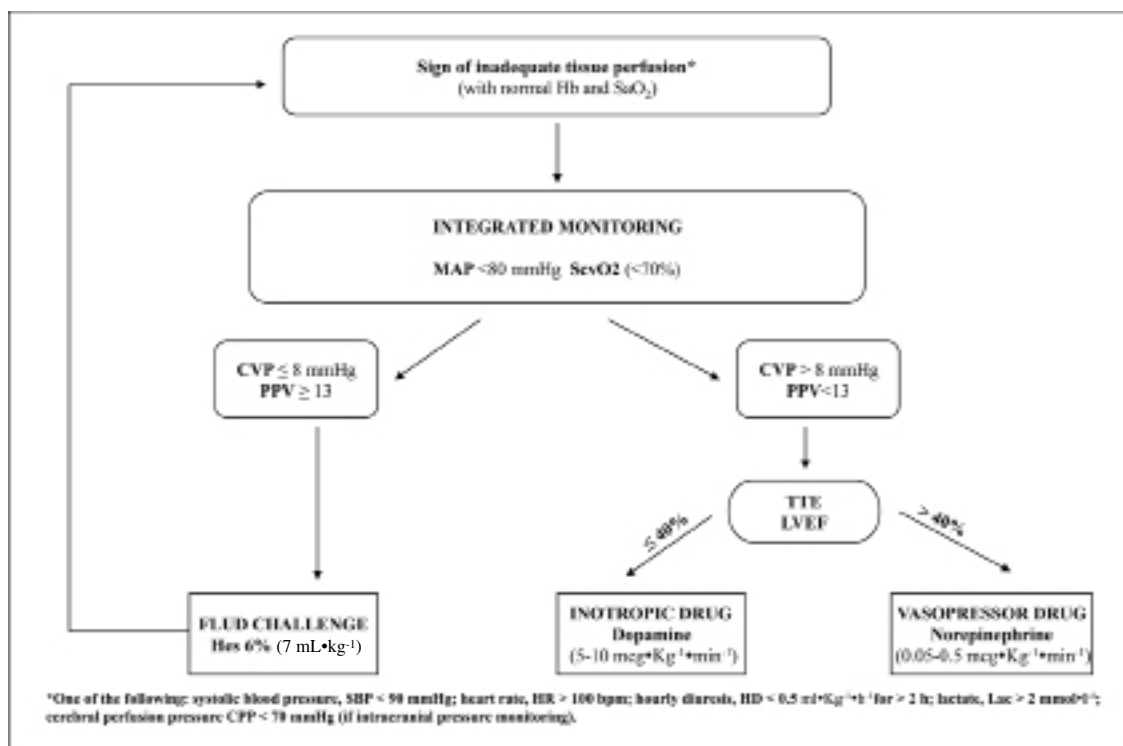


Figure 1.—Local guidelines for haemodynamic management of critically ill patients.

Hb: hemoglobin; SaO<sub>2</sub>: arterial oxygen saturation; MAP: mean arterial pressure; ScvO<sub>2</sub>: central venous oxygen saturation; CVP: central venous pressure; PPV: pulse pressure variation; TTE: transthoracic echocardiography; LVEF: left ventricular ejection fraction; Hes: hydroxyethylstarch.

\*One of the following: systolic blood pressure, SBP < 90 mmHg; heart rate, HR > 100 bpm; hourly diuresis, HD < 0.5 mL/kg/h for > 2 h; lactate, Lac > 2 mmol/L; cerebral perfusion pressure CPP < 70 mmHg (if intracranial pressure monitoring).

to-noise ratio.<sup>9</sup> No therapeutic intervention was based on the CO values provided by MostCare.

### Study intervals and experimental procedure

After ICU admission and stabilization, TTE-CO and MC-CO were recorded simultaneously before the physician decided to perform one of the therapeutic interventions aimed at hemodynamic optimization. Thereafter measurements were made at the end of the fluid challenge or 30 minutes after vasopressors initiation, in the presence of stable MAP (less than 10% variation over 15 minutes). For each measurement of TTE-CO, a corresponding value from the MostCare monitor was obtained by averaging the individual stroke volumes over the time needed for each TTE-CO measurement. These values were automatically downloaded and recorded in a computer database for off-line analysis.

### Statistical analysis

Statistical analysis was performed using StatsDirect version 2.5.8 (Cheshire, UK), SigmaPlot for Windows version 11.0 (Systat Software, Inc., San Jose, CA) and R version 2.11.1 (2010-05-31 R Foundation for Statistical Computing, Vienna, Austria).<sup>16</sup> We calculated that at least 44 patients would be required assuming to allow differences in the average between the two methods of 0.5 L/min and to have a standard deviation of 1 L/min; we considered a statistical significance level of 95% ( $\alpha=0.05$ ) and a minimum power of 90% ( $\beta=0.1$ ). The agreement between TTE-CO and MC-CO was assessed using the Bland-Altman method.<sup>17</sup> The correlation coefficient, bias and their 95% CI (mean difference between measurements) were calculated. Limits of agreement (LoA) (as 2.2 times SD of the bias) were computed as proposed by Ludbrook for small

samples.<sup>18</sup> The 95% CI of the upper LoA and that of the lower LoA were also calculated. The percentage of error was calculated as the limits of agreement (2.2 times the SD of the bias) divided by the mean CO from the two methods, as proposed by Critchley:  $100 \times (2.2 \times \text{SD of Bias}) / [(\text{mean}_{\text{TTE-CO}} + \text{mean}_{\text{MC-CO}}) / 2]$ .<sup>19</sup>

Changes ( $\Delta$ ) in CO were calculated for the group of patients with two CO determinations (baseline and after fluid challenge) and three CO determinations (baseline, T1; after fluid challenge, T2; after the start of norepinephrine infusion, T3) by subtracting the first from the second measurement (T2-T1) and the second from the third (T3-T2) when present. We used the method suggested by Myles and Cui to adjust for the effects of repeated measurements in the Bland-Altman analysis.<sup>20</sup> For this purpose, and also to test changes of TTE-CO and MC-CO at the different phases, we used the method that was applied in previous studies.<sup>21-23</sup>

The ability of the MostCare to reliably follow changes or trends in CO was assessed using a concordance analysis.<sup>24</sup> After excluding all the pairs of  $\Delta$ CO where at least one value was zero, the direction of change between TTE-CO and MC-CO was analyzed to assess the percentage of concordance between the results, including and excluding  $\Delta$ TTE-CO  $< 0.5 \text{ L} \cdot \text{min}^{-1}$ .<sup>25</sup> The serial pairs of CO readings from the echocardiographic method (X-axis) and the MostCare system (Y-axis) were converted to polar coordinates and the resulting polar plots were used to show trending ability.<sup>26, 27</sup> This was based on the percentage of data points lying within 30-degrees of the polar axis.<sup>27</sup> For all statistical tests, a  $P < 0.05$  was taken to indicate significance.

## Results

Patients' characteristics are described in Table I. All patients had blunt trauma and no patient had diagnosis of intra-abdominal hypertension or abdominal compartment syndrome. One hundred sixteen paired CO values were obtained. TTE-CO values ranged from 2.9 to 7.6  $\text{L} \cdot \text{min}^{-1}$ , and MC-CO ranged from 2.8 to 8.2  $\text{L} \cdot \text{min}^{-1}$ . Forty-one patients (group A) received a fluid challenge; in 18 of them (Group B), norepinephrine

TABLE I.—Patients' characteristics. Data are expressed as mean  $\pm$  standard deviation [range]. SAPS II, Simplified Acute Physiological Score II; ICP, intracranial pressure.

	N.=49
Age (yr)	52 $\pm$ 23 [19-79]
Gender (male/female)	30/19
Weight (kg)	75 $\pm$ 12
Height (cm)	172 $\pm$ 13
Body surface area (kg/m <sup>2</sup> )	1.78 $\pm$ 0.29
SAPS II	32 [28-40]
ICP (mmHg)	30
District of trauma	
Head	30
Chest	19
Pelvis	4
Limb	12
Rachis	5
Abdomen	2

infusion was started thereafter. Eight patients with severe traumatic brain injury (Group C) were treated with norepinephrine infusion only, to maintain adequate cerebral perfusion pressure. No patient received inotropes. Among the various hemodynamic variables, CO and MAP showed a significant change after fluid challenge or norepinephrine infusion ( $P < 0.05$ ) (Table II).

In the group A, we found a good correlation between TTE-CO and MostCare-CO ( $r = 0.94$ , 95% CI = 0.92 to 0.97,  $P < 0.001$ ) at baseline. Mean bias was  $-0.06 \text{ L} \cdot \text{min}^{-1}$  with LoA of  $-0.74$  to  $0.62 \text{ L} \cdot \text{min}^{-1}$  (lower 95% CI,  $-0.93$  to  $-0.56$ ; upper 95% CI,  $0.44$  to  $0.81$ ) and a relative percentage error (PE) of 14.1% (Table III). For those patients in which norepinephrine infusion was subsequently initiated (group B), similar values of  $r$ , mean bias, and PE were observed (Table III). In the group C, the correlation at baseline was 0.94 (95% CI = 0.72 to 0.99,  $P < 0.001$ ), the mean bias was  $-0.06 \text{ L} \cdot \text{min}^{-1}$  with LoA of  $-0.79$  to  $0.67 \text{ L} \cdot \text{min}^{-1}$  (lower 95% CI,  $-1.23$  to  $-0.34$ ; upper 95% CI,  $0.22$  to  $1.11$ ) and a PE of 18.2% (Table III). After the start of norepinephrine infusion, the correlation was comparable to the baseline results (Table III).

The mean bias for all 116 CO measurements corrected for repeated measures was  $-0.06 \text{ L} \cdot \text{min}^{-1}$  with LoA of  $-0.94$  to  $0.82 \text{ L} \cdot \text{min}^{-1}$  (lower 95% CI,  $-1.16$  to  $-0.72$ ; upper 95% CI,  $0.60$  to  $1.04$ ) and a PE of 17.7% (Figure 2A). The correlation was statistically significant ( $r = 0.94$ ,

TABLE II.—Hemodynamic data recorded at each time-point of the study. Group A: patients who received fluid challenge only. Group B: patients who received norepinephrine after a fluid challenge. Group C: patients treated with norepinephrine only. Data are expressed as mean (standard deviation, SD). HR: heart rate; MAP: mean arterial pressure; CVP: central venous pressure; MC-CO: continuous cardiac output obtained by MostCare; TTE-CO: cardiac output obtained by Transthoracic Echocardiography technique.

Variable	Group A (N.=41)			Group B (N.=18)			Group C (N.=8)		
	Baseline	Fluid challenge	P value	Baseline 2*	Norepinephrine	P value	Baseline	Norepinephrine	P value
HR (min <sup>-1</sup> )	83±17	81±17	0.001	86±14	88±21	0.50	81±12	78±11	0.056
MAP (mmHg)	86.3±12	89.5±12	0.001	83.0±14	88.0±8	0.27	70.6±7	85.4±6	0.01
CVP (mmHg)	7.7±3	9.5±2	0.001	8.0±2.2	9.8±3	0.09	10.6±3	11.4±2	0.06
Volume Load (mL)	—	490±50	—	—	—	—	—	—	—
Norepinephrine (mcg·kg <sup>-1</sup> ·min <sup>-1</sup> )	—	—	—	—	0.19±0.12	—	—	0.27±0.08	—
MC-CO (L·min <sup>-1</sup> )	4.88±1.02	5.34±1.03	0.001	5.38±0.68	5.22±0.82	0.27	4.02±0.73	4.32±0.75	0.10
TTE-CO (L·min <sup>-1</sup> )	4.81±0.95	5.33±0.98	0.001	5.40±0.81	5.09±0.86	0.43	3.96±0.91	4.26±0.78	0.09

\*After fluid challenge, before receiving norepinephrine.

TABLE III.—Mean differences between TTE-CO and MC-CO (bias and 95% confidence interval, CI). Limits of agreement (LoA) were computed as proposed by Ludbrook for small samples (i.e., 2.2 times standard deviations of the bias). Percentage error (PE) and coefficient of correlation (r) are calculated for cardiac output measurements at different times. Data are expressed as count, percentage, and mean ± standard deviation (SD). Group A: patients who received fluid challenge. Group B: patients who received fluid challenge plus norepinephrine. Group C: patients treated with only norepinephrine.

Group	time	Bias (95% CI) (L·min <sup>-1</sup> )	LoA	95% CI of lower LoA	95% CI of upper LoA	PE (%)	r
A plus B	Baseline (N.=41)	-0.06 (-0.17 to -0.05)	-0.74 to 0.62	-0.93 to -0.56	0.44 to 0.81	14.1	0.94
	Fluid challenge (N.=41)	-0.01 (-0.12 to 0.10)	-0.71 to 0.69	-0.90 to -0.52	0.50 to 0.88	13.2	0.87
	Norepinephrine (N.=18)	-0.14 (-0.36 to 0.08)	-1.09 to 0.81	-1.47 to -0.70	0.42 to 1.19	18.4	0.86
C	Baseline (N.=8)	-0.06 (-0.32 to 0.20)	-0.79 to 0.67	-1.23 to -0.34	0.22 to 1.11	18.2	0.94
	Norepinephrine (N.=8)	-0.06 (-0.29 to 0.17)	-0.72 to 0.60	-1.12 to -0.32	0.20 to 1.00	15.4	0.91
All data		-0.06 (-0.19 to 0.07)	-0.94 to 0.82	-1.16 to -0.72	0.60 to 1.04	17.7	0.94

95% CI=0.89 to 0.97; P<0.001). The mean differences between TTE-CO and MostCare-CO together with 95% limits of agreement and their corresponding 95% CI, and the mean percentage error are shown in Table III.

$\Delta$ CO was calculated separately for the two methods. Data comparison showed a correlation of 0.91 (95% CI=0.87 to 0.95; P<0.001) (Figure 2B) and a bias of -0.01 L·min<sup>-1</sup> with LoA of -0.67 to 0.65 L·min<sup>-1</sup> (lower 95% CI, -0.83 to -0.51; upper 95% CI, 0.48 to 0.81).

Five  $\Delta$ CO pairs were excluded from the analysis of the direction of changes, as  $\Delta$ CO value was zero. The concordance of  $\Delta$ CO observed was 90% (56 of 62 pairs of  $\Delta$ CO agreed); when

only  $\Delta$ TTE-CO >0.5 L·min<sup>-1</sup> were considered, the concordance improved to 97% (36/37). A polar plot was used to show the direction of CO changes (i.e., trending ability) (Figure 3A). The polar plot analysis confirmed good agreement and good concordance for  $\Delta$ CO estimated by the two devices. Indeed, 100% of data points lied within 30-degrees of the polar axis. The mean polar angle was 0.3-degrees, with the radial limits of agreement of 348 to 12 (Figure 3B).

## Discussion

In the present study, for the first time the MostCare system was compared to TTE during

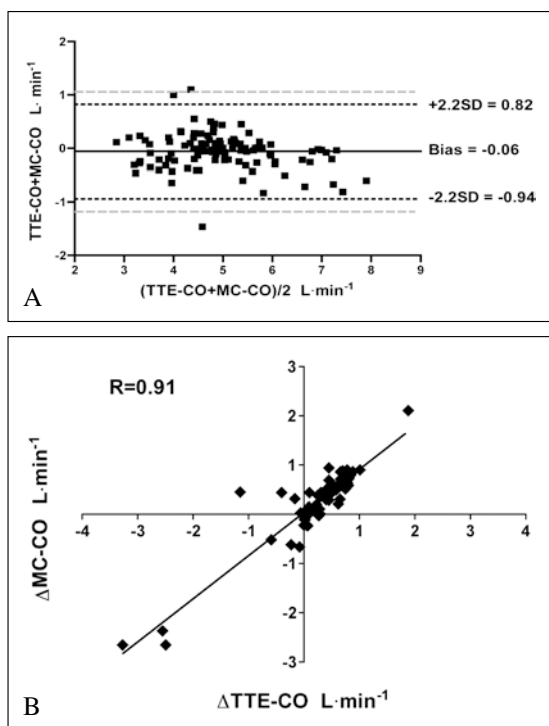


Figure 2.—A) Bland-Altman plots of cardiac output (CO) estimated by transthoracic echocardiography (TTE-CO) and by MostCare (MC-CO) for all 116 paired data. The mean bias was  $-0.06$  with limits of agreement of  $-0.94$  to  $0.82$   $L \cdot \text{min}^{-1}$ . Solid line, mean difference (bias); dashed black lines, limits of agreement (bias  $\pm 2.2$  SD). Dashed gray lines, 95% confidence interval of limits of agreement. B) Four-quadrant trend plot showing the relationship between changes ( $\Delta$ ) in cardiac output (CO) estimated by transthoracic echocardiography (TTE-CO) and by MostCare (MC-CO).  $\Delta$  in CO were calculated by subtracting the first from the second measurement (T2-T1), and the second from the third (T3-T2) when it was required. Correlation coefficient ( $r$ ) was equal to  $0.91$  (95% confidence interval [CI]= $0.89$  to  $0.97$ ;  $P < 0.001$ ).

interventions aimed at optimizing hemodynamics in trauma patients. MostCare provided good agreement with echocardiography, showing a percentage of error lower than 30%, which is considered as the limit for clinical acceptance for a new method.<sup>19</sup> Furthermore, good agreement in detecting changes in CO ( $\Delta$ CO) was found either after fluid challenge or vasopressor therapy.

Our analytical approach included both Bland-Altman and polar plot analyses. Bland-Altman analysis has been widely used to evaluate the accuracy of CO-monitoring devices; also, the direction of changes and the correlation analysis

were the only statistical methods available to assess the ability of a device to detect the changes in CO after therapeutic interventions. In this setting, polar plots analysis is a new statistical approach to detect CO changes over time between two monitoring techniques. The polar plot analysis quantifies CO changes (the so-called “trending ability”) by converting the serial pairs of CO readings from the reference method (in this case, TTE, on X-axis) and the other method (here, MostCare system, Y-axis) to polar coordinates. The mean change in cardiac output ( $\Delta$ CO) is shown by the distance from the center of the plot and the agreement is indicated by the angle with the horizontal axis. Thus, the better the agreement between CO measurements, the closer the data pairs will be to the horizontal axis. The dotted lines represent the limits of good agreement ( $\pm 0.5$   $L/\text{min}$ ); in this plot, no data-points lie outside these limits, showing the good trending ability of the MostCare system (Figure 3).

Due to its invasiveness and potential complications, the use of PAC is actually not recommended in all trauma patients, but it is limited to selected patient populations.<sup>4</sup> Echocardiography can overcome the limitations of PAC and represents a useful diagnostic device for early hemodynamic assessment in trauma patients. On the other hand, it cannot eliminate the need for continuous monitoring and for the early recognition of abrupt hemodynamic alterations.<sup>1, 5, 6</sup> PCMs may obviate the limitations of PAC and may complement echocardiography in the hemodynamic evaluation and management of critically ill patients.<sup>28</sup> Among all PCMs, the MostCare system is a device that allows beat-to-beat CO measurement.<sup>7, 8</sup> A number of papers confirm the reliability of MostCare during various hemodynamic scenarios and in different patient populations.<sup>8-11, 23, 29</sup> Our results showed similar agreement of MC-CO with CO measured with standard techniques, such as TTE and PAC, in previous studies and suggested that this uncalibrated PCM may be a reliable tool to assess CO also in hemodynamically stable trauma patients.

Previous studies have already compared MostCare with echocardiography. Romagnoli *et al.*<sup>9</sup> showed good agreement between CO measured

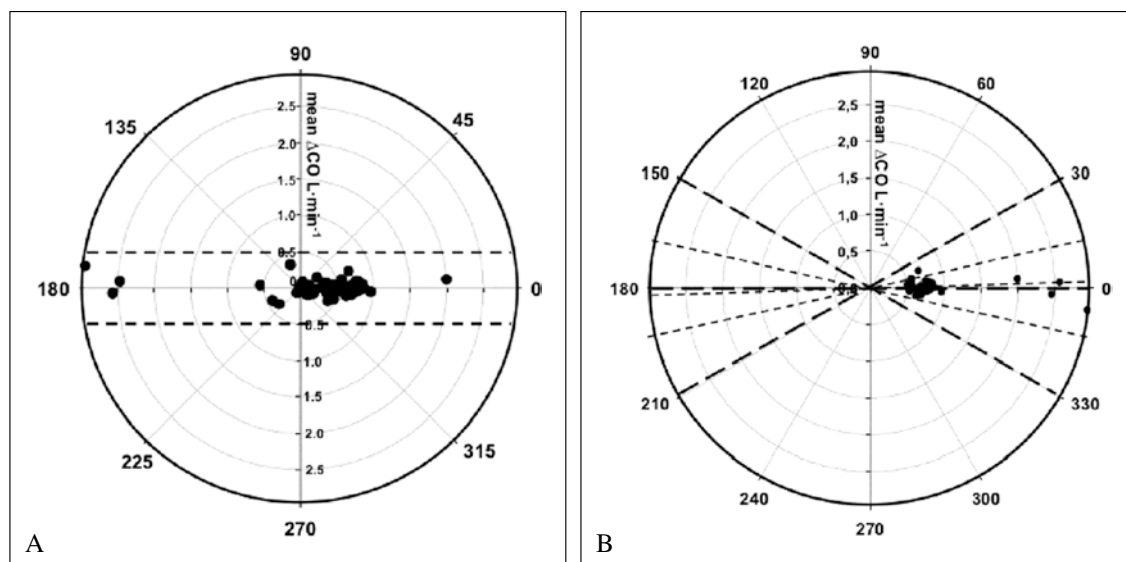


Figure 3.—A) Polar plot shows the direction of CO changes (trending ability). This was obtained by converting the serial pair of CO readings from TTE method (X-axis) and MostCare system (Y-axis) to polar coordinates.<sup>26</sup> The dotted lines represent the limits of good agreement ( $\pm 0.5$  L·min<sup>-1</sup>) and the distance from the center of the plot represents the mean change in cardiac output ( $\Delta$ CO). The better the agreement between CO measurements, the closer data pairs will lie along the horizontal axis. In this plot, no data points lie outside these limits, showing the good trending ability of the MostCare system. B) Polar plot designed to include the analysis of the mean polar angle and the radial limits of agreement. In this new polar plot, proposed by Critchley et al,<sup>27</sup> the radial limits of agreement are based on the 95% confidence limits of the polar angle. The mean polar angle gives insight into how well the calibration of the two devices being compared, test and reference methods, agree. Dashed lines show polar axis (e.g. horizontal axis: 0-degree) and  $\pm 30$ -degree axes. The later coincide with the benchmark 30-degree limits for acceptable trending ability. Dotted lines show mean and 95% confidence intervals for the data or polar angles. In this plot, acceptable trending ability is present as 100% of data points lies within 30-degrees of the polar axis.

by MostCare and by transesophageal echocardiography in pigs during several hemodynamic scenarios, including dobutamine infusion, vasopressor therapy and fluid loading. Nevertheless, a percentage of error greater than 30%, suggesting poor agreement, was observed during severe haemorrhage, defined by a reduction of blood volume  $\geq 35\%$ . This limitation of MostCare should be taken into account whenever such device is used to monitor CO in trauma patients with severe bleeding. However, as no human studies have been performed using MostCare under these circumstances, further investigations are needed to define the accuracy of this PCM to measure CO in critically ill patients with concomitant severe blood loss.

Calamandrei *et al.*<sup>11</sup> studied the MostCare system in a pediatric population (aged between 1 month and 18 years old). They found that MostCare provided reliable estimation of CO when compared with TTE. Although the authors en-

rolled a large cohort of patients, no therapeutic interventions was used to change CO and only stable hemodynamic conditions were analyzed.

Other PCMs devices were compared with echocardiography in critically ill patients.<sup>13, 30-32</sup> The Pulse Contour Cardiac Output (PCCO) system (Medical Systems AG, Munich, Germany) was compared with echocardiography for the evaluation of left ventricle systolic function<sup>31</sup> and dynamic index of preload.<sup>32</sup> The PCCO device works differently than MostCare because it needs a dedicated arterial catheter with a thermistore in its tip and a calibration with thermodilution. Several studies showed the reliability of the PCCO system in various clinical settings,<sup>33, 34</sup> including cardiac surgery and sepsis, however none of them was conducted in trauma patients.

The Vigileo monitor (Edwards Lifesciences, Irvine, CA, USA) is another widely used PCM device that proved to be reliable in a number

of scenarios.<sup>13, 30</sup> Vigileo and echocardiography were compared by Concha and colleagues,<sup>30</sup> who didn't find any good agreement between the two techniques in a population of low risk patients undergoing laparoscopic colon surgery. The authors supposed that the variations of patient's position (*i.e.*, supine lithotomy position, Trendelenburg, reverse Trendelenburg, and steep Trendelenburg position), as well as the induced pneumoperitoneum related to the laparoscopic procedure, may have determined major changes in vascular compliance and impedance which may have contributed to the discrepancy between echocardiography and Vigileo.<sup>30</sup>

MostCare is powered by PRAM (Pressure Recording Analytical Method) that has been validated in different clinical scenarios.<sup>7-11, 23, 29</sup> With PRAM the systemic impedance is determined by the physical characteristics of the circulatory system of the subject under study.<sup>7, 8</sup> Thus, changes in vascular tone should influence to a lesser extent the reliability of MostCare in measuring CO. This statement was recently confirmed in a small group of septic patients in which changes in vascular tone were induced by norepinephrine infusion.<sup>29</sup>

Several limitations of the MostCare system remain to be addressed. Either over- or underdamped arterial pressure waveforms may affect the precision of the pressure wave analysis.<sup>35, 36</sup> Also, the adequate analysis of the blood pressure wave at 1000 Hz is dependent from the operator, who needs to maximize the quality of the arterial signal to obtain a reliable pressure wave morphology.<sup>7, 9, 37</sup>

Moreover, the characteristics of the arterial tree (such as stenosis, aortic valve and ascending aorta pathologies, etc.) could influence the accuracy of CO measurements based on the analysis of the arterial waveform.<sup>28, 36</sup> Also, cardiac dysrhythmias, especially atrial fibrillation, can affect the reliability of MostCare whenever comparing it to PAC-derived CO or other hemodynamic monitoring techniques.<sup>38</sup> The presence of some of these factors may explain why some authors found a weak correlation between MostCare and the thermodilution method.<sup>39</sup> Notably, all the aforementioned conditions were considered as exclusion criteria in the present study and ac-

counted for the good agreement that we found between the two techniques.

Some limitations of the present study have to be addressed. First, we did not compare MostCare with bolus thermodilution (ThD), which is considered the gold standard method to estimate CO in clinical practice. Actually, MostCare has already been shown good agreement in estimating CO when compared to ThD under different clinical conditions, including cardiac surgery, use of intra-aortic balloon pump conterpulsation and other mechanical assist devices, and sepsis.<sup>8, 23, 29, 40</sup> Also, since echocardiography is widely used in critically ill patients as a valued alternative to ThD to estimate CO, it could be reasonable to consider such a technique as a valid reference tool for CO comparison in this setting. Second, MostCare is one of the last devices proposed for minimal invasive hemodynamic monitoring. It has been developed in Italy a few years ago and its clinical validation, even if quite convincing, suffers the paucity of specific studies performed outside Italian centers. Indeed, two recent articles from other groups have raised some concerns on the feasibility of this device.<sup>39, 41</sup> An ongoing multicenter study, involving several European centers, will hopefully provide more information on the value of MostCare in critically ill patients. Third, we did not analyse other possible hemodynamic changes in addition to fluid challenge and norepinephrine infusion (*e.g.*, severe haemorrhage, inotrope administration or blood transfusions). Moreover, measurements were performed only after initial resuscitation and during stable hemodynamic conditions. Hence, further larger studies are needed to confirm these data in other phases of trauma management. Finally, the decisional algorithm used in this study to treat trauma patients with fluids and/or vasopressors could be largely criticized. In trauma with haemorrhagic shock, the aim of restoring normal blood pressure during the active bleeding phase, as well as fluid management based on PPV, have been questioned and there is not much agreement on hemodynamic goals for pre-definitive care, which may vary in relation to the injured organ. Thus, the protocol followed in the present study may not be applicable to all trauma subsets. Nevertheless, the aim



of this study was not to propose (or to validate) a specific management protocol to treat trauma patients but only to evaluate the MostCare accuracy in tracking CO changes before and after therapeutical interventions.

### Conclusions

Under the studied conditions MostCare showed a good agreement with echocardiography over a wide range of CO. Echocardiography and pulse contour methods should be considered complementary in monitoring hemodynamics in critically ill patients. Indeed, echocardiography can provide relevant "diagnostic" information, while pulse contour methods represent useful beat-to-beat "monitoring" tools to assess patients' hemodynamic variations.<sup>42</sup> This is particularly important in trauma subjects, for whom invasive hemodynamic monitoring techniques are often deemed harmful or not essential for clinical management.

### Key messages

— MostCare showed good agreement with echocardiography to measure cardiac output in trauma patients, after initial hemodynamic stabilization.

— In such patients, pulse contour analysis by MostCare device could also accurately detect hemodynamic changes induced by fluids and/or vasopressors administration.

— Further studies are needed to evaluate the accuracy of MostCare to detect hemodynamic changes in unstable trauma patients.

### References

1. Kohli-Seth R, Neuman T, Sinha R, Bassily-Marcus A. Use of echocardiography and modalities of patient monitoring of trauma patients. *Curr Opin Anaesthesiol* 2010;23:239-45.
2. Vincent JL, Pinsky MR, Sprung CL, Levy M, Marini JJ, Payen D *et al.* The pulmonary artery catheter: in medio virtus. *Crit Care Med* 2008;36:3093-6.
3. Bein B, Worthmann F, Tonner PH, Paris A, Steinfath M, Hedderich J *et al.* Comparison of Esophageal Doppler, Pulse Contour Analysis, and Real-Time Pulmonary Artery Thermomodulation for the Continuous Measurement of Cardiac Output. *J Cardiothorac Vasc Anesth* 2008;18:185-9.
4. Barmparas G, Inaba K, Georgiou C, Hadjizacharia P, Chan

5. Cheitlin MD, Armstrong WF, Aurigemma GP, Beller GA, Bierman FZ, Davis JL *et al.* ACC/AHA/ASE Guideline Update for the Clinical Application of Echocardiography: A Report of the American College of Cardiology/American Heart. *J Am Soc Echocardiogr* 2003;16:1091-110.
6. Vignon P. Hemodynamic assessment of critically ill patients using echocardiography Doppler. *Curr Opin Crit Care* 2005;11:227-34.
7. Romano SM, Pistolesi M. Assessment of cardiac output from systemic arterial pressure in humans. *Crit Care Med* 2002;30:1834-41.
8. Giomarelli P, Biagioli B, Scolletta S. Cardiac output monitoring by pressure recording analytical method in cardiac surgery. *Eur J Cardiothorac Surg* 2004;26:515-20.
9. Romagnoli S, Romano SM, Bevilacqua S, Ciappi F, Lazzeri C, Paris A *et al.* Cardiac output by arterial pulse contour: reliability under hemodynamic derangements. *Interact Cardiovasc Thorac Surg* 2009;8:642-6.
10. Scolletta S, Romano SM, Biagioli B, Capannini G, Giomarelli P. Pressure recording analytical method (PRAM) for measurement of cardiac output during various hemodynamic states. *Br J Anaesth* 2005;95:159-65.
11. Calamandrei M, Mirabile L, Muschetta S, Gensini GF, De Simone L, Romano SM. Assessment of cardiac output in children: a comparison between the pressure recording analytical method and Doppler echocardiography. *Pediatr Crit Care Med* 2008;9:310-2.
12. Vincent JL, Weil MH. Fluid challenge revisited. *Crit Care Med* 2006;34:1333-7.
13. Biais M, Vidil L, Sarabay P, Cottenceau V, Revel P, Sztark F. Changes in stroke volume induced by passive leg raising in spontaneously breathing patients: comparison between echocardiography and Vigileo/FloTrac device. *Crit Care* 2009;13:R195.
14. Kleinman B, Powell S, Kumar P, Gardner RM. The fast flush test measures the dynamic response of the entire blood pressure monitoring system. *Anesthesiology* 1992;77:1215-20.
15. Michard F, Boussat S, Chemla D, Anguel N, Mercat A, Lecarpentier Y *et al.* Relation between respiratory changes in arterial pulse pressure and fluid responsiveness in septic patients with acute circulatory failure. *Am J Respir Crit Care Med* 2000;162:134-8.
16. R Development Core Team. R: A language and environment for statistical computing R Foundation for Statistical Computing, Vienna, Austria [Internet]. Available at <http://www.R-project.org> [cited 2012, Dec 13].
17. Bland JM, Altman DG. Statistical methods for assessing agreement between two methods of clinical measurement. *Lancet* 1986;1:307-10.
18. Ludbrook J. Statistical techniques for comparing measurers and methods of measurement: a critical review. *Clin Exp Pharmacol Physiol* 2002;29:527-36.
19. Critchley LAH, Critchley JA. A meta-analysis of studies using bias and precision statistics to compare cardiac output measurement techniques. *J Clin Monitor* 1999;15:85-91.
20. Myles PS, Cui J. Using the Bland-Altman method to measure agreement with repeated measures. *Br J Anaesth* 2007;99:309-11.
21. Carstensen B, Simpson J, Gurrin L. Statistical models for assessing agreement in method comparison studies with replicate measurements [Internet]. Available at: <http://staff.pubhealth.ku.dk/~bxc/MethComp/lam-bsa.pdf> [cited 2008, Jun 7].
22. Carstensen B, Gurrin L. MethComp: Functions for analysis of method comparison studies. R package version 1.2-1 [Internet]. Available at: <http://www.pubhealth.ku.dk/~bxc/MethComp/introMethComp.pdf> [cited 2010, Jan 8].

23. Scolletta S, Franchi F, Taccone FS, Donadello K, Biagioli B, Vincent JL. An uncalibrated pulse contour method to measure cardiac output during aortic counterpulsation. *Anesth Analg* 2011;113:1389-95.
24. Biancofiore G, Critchley LAH, Lee A, Bindi L, Bisà M, Esposito M *et al.* Evaluation of an uncalibrated arterial pulse contour cardiac output monitor system in cirrhotic patients undergoing liver surgery. *Br J Anaesth* 2009;102:47-54.
25. Jansen JR, Schreuder JJ, Mulier JP, Smith NT, Settels JJ, Wesseling KH. A comparison of cardiac output derived from the arterial pressure wave against thermodilution in cardiac surgery patients. *Br J Anaesth* 2001;87:212-22.
26. Critchley LA, Lee A, Ho AM. A critical review of the ability of continuous cardiac output monitors to measure trends in cardiac output. *Anesth Analg* 2010;111:1180-92.
27. Critchley LA, Yang XX, Lee A. Assessment of trending ability of cardiac output monitors by polar plot methodology. *J Cardiothorac Vasc Anesth* 2011;25:536-46.
28. Alhashemi JA, Cecconi M, Hofer CK. Cardiac output monitoring: an integrative perspective. *Crit Care* 2011;15:214.
29. Franchi F, Silvestri R, Cubattoli L, Taccone FS, Donadello K, Romano SM *et al.* Comparison between an uncalibrated pulse contour method and thermodilution technique for cardiac output estimation in septic patients. *Br J Anaesth* 2011;107:202-8.
30. Concha MR, Mertz VF, Cortínez LI, González KA, Butte JM. Pulse contour analysis and transesophageal echocardiography: a comparison of measurements of cardiac output during laparoscopic colon surgery. *Anesth Analg* 2009;109:114-8.
31. Combes A, Berneau JB, Luyt CE, Trouillet JL. Estimation of left ventricular systolic function by single transpulmonary thermodilution. *Intensive Care Med* 2004;30:1377-83.
32. Rex S, Brose S, Metzelder S, Hüneke R, Schälte G, Autschbach R *et al.* Prediction of fluid responsiveness in patients during cardiac surgery. *Br J Anaesth* 2004;93:782-8.
33. Rödig G, Prasser C, Keyl C, Liebold A, Hobbhahn J. Continuous cardiac output measurement: pulse contour analysis vs thermodilution technique in cardiac surgical patients. *Br J Anaesth* 1999;82:525-30.
34. Monnet X, Anguel N, Naudin B, Jabot J, Richard C, Teboul JL. Arterial pressure-based cardiac output in septic patients: different accuracy of pulse contour and uncalibrated pressure waveform devices. *Crit Care* 2010;14:R109.
35. Gibbs N, Gardner RM. Dynamics of invasive pressure monitoring systems: clinical and laboratory evaluation. *Heart Lung* 1988;17:43-51.
36. Camporota L, Beale R. Pitfalls in haemodynamic monitoring based on the arterial pressure waveform. *Crit Care* 2010;14:124.
37. Scolletta S, Taccone FS, Romagnoli S, Landoni G, Giomarelli P. The pressure recording analytical method (PRAM) to measuring cardiac output after cardiac surgery: some practical considerations. *Br J Anaesth* 2011;107:814-5.
38. Maj G, Monaco F, Landoni G, Maj G, Monaco F, Landoni G *et al.* Cardiac Index Assessment by the Pressure Recording Analytic Method in Unstable Patients With Atrial Fibrillation. *J Cardiothorac Vasc Anesth* 2011;25:476-80.
39. Paarmann H, Groesdonk HV, Sedemund-Adib B, Hanke T, Heinze H, Heringlake M *et al.* Lack of agreement between pulmonary arterial thermodilution cardiac output and the pressure recording analytical method in postoperative cardiac surgery patients. *Br J Anaesth* 2011;106:475-81.
40. Scolletta S, Miraldi F, Romano SM, Muzzi L. Continuous cardiac output monitoring with an uncalibrated pulse contour method in patients supported with mechanical pulsatile assist device. *Interact Cardiovasc Thorac Surg* 2011;13:52-6.
41. Biais M, Cottenceau V, Stecken L, Jean M, Ottolenghi L, Roulet S *et al.* Evaluation of stroke volume variations obtained with the pressure recording analytic method. *Crit Care Med* 2012;40:1186-91.
42. Vincent JL, Rhodes A, Perel A, Martin GS, Della Rocca G, Vallet B *et al.* Clinical review: Update on hemodynamic monitoring--a consensus of 16. *Crit Care* 2011;18:15:229.

*Conflicts of interest.*—Sabino Scolletta has received from Vygon lecture fees, research grants and some material for clinical studies. Federico Franchi, Katia Donadello and Pierpaolo Giomarelli have received from Vygon some material for studies.

Received on February 13, 2012 - Accepted for publication on September 18, 2012.

Corresponding author: F. Franchi, Department of Anesthesia and Intensive Care Unit, University of Siena, Viale Bracci 1, 53100 Siena, Italy. E-mail: franchif@unisi.it